

Biotin 3' End DNA Labeling Kit

89818

1290.6

Number	Description
89818	<p>Biotin 3' End DNA Labeling Kit, sufficient reagents to perform 20 labeling reactions (5 pmol each)</p> <p>Kit contents:</p> <p>5X TdT Reaction Buffer, 1mL, 500mM cacodylic acid, 10mM CoCl₂, 1mM DTT, pH 7.2; store at -20°C.</p> <p>Terminal Deoxynucleotidyl Transferase (TdT), 50µL; ~20 U/µL in 100mM potassium phosphate, 10mM 2-mercaptoethanol, 50% glycerol, pH 6.9; store at -20°C</p> <p>Biotin-11-UTP, 100µL; 5µM in 10mM Tris•HCl, 1mM EDTA, pH 7.5; store at ≤ 4°C and minimize freeze-thaw cycles and exposure to light</p> <p>Unlabeled Control Oligo, 140µL; 1µM in 10mM Tris•HCl, 1mM EDTA, pH 7.5; store at -20°C</p> <p>Biotin-Control Oligo, 40µL; 1µM in 10mM Tris•HCl, 1mM EDTA, pH 7.5; store at -20°C</p>

Storage: Upon receipt store individual components as indicated. Product is shipped with dry ice.

Table of Contents

Introduction	1
Labeling Procedure	2
Procedures for Estimating Labeling Efficiency	3
Related Pierce Products	5
Appendix	5
Cited References	5
Product Reference	5

Introduction

The Thermo Scientific Biotin 3' End DNA Labeling Kit uses TdT to incorporate 1-3 biotinylated ribonucleotides onto the 3' end of DNA strands. This labeling strategy has the advantage of localizing the biotin to the 3' end of the probe where it is less likely to interfere with hybridization or sequence-specific binding of proteins. Biotin-labeled DNA probes can be used to facilitate non-isotopic detection in a variety of applications including electrophoretic mobility shift assays (EMSA), Northern or Southern blots, colony hybridizations, or *in situ* hybridizations.

The enzyme terminal deoxynucleotidyl transferase (TdT) catalyzes non-template-directed deoxynucleotide incorporation onto the 3'-OH end of DNA.¹⁻² TdT exhibits substrate preference for single-stranded DNA, but it will also label duplex DNA with 3' overhangs and blunt duplexes, albeit with lower efficiency.³ Under the appropriate conditions (in the presence of Co²⁺), TdT will incorporate ribonucleotides onto the 3' end of DNA as well.²

For nonisotopic EMSA applications, use the Thermo Scientific LightShift Chemiluminescent EMSA Kit (Product No. 20148). For nonisotopic Northern or Southern blotting applications, use the Thermo Scientific North2South Chemiluminescent Nucleic Acid Hybridization and Detection Kit (Product No. 17097). For other types of nucleic acid detection by means of the biotin-labeled DNA probe, use the Chemiluminescent Nucleic Acid Detection Module (Product No. 89880).

Labeling Procedure

Note: This procedure is optimized for labeling 5 pmol of 3'-OH ends in each reaction. The presence of Mg²⁺, protein and residual agarose may decrease labeling efficiency. Use only purified DNA in the following reaction. For applications requiring double-stranded DNA oligos, end-label both complementary oligonucleotides separately and then anneal them before use (see note after Step B.8).

A. Additional Materials Required

- Ultrapure water
- 1 μM of oligonucleotide for labeling
- 37°C heat block or water bath
- 0.2M EDTA, pH 8.0
- Chloroform:isoamyl alcohol (24:1)
- Microcentrifuge tubes and microcentrifuge

B. Labeling Reaction

1. Thaw all kit components except the TdT, and place them on ice. Keep TdT at -20°C until needed.
2. Just before use, dilute a portion of the TdT stock in 1X TdT Reaction Buffer to a working concentration of 2 U/μL. For example, prepare enough diluted TdT for each reaction by combining 2 μl of 5X TdT Reaction Buffer, 7 μL of ultrapure water and 1 μL of 20 U/μL stock of TdT.

Note: Use the diluted TdT stock immediately. Do not store the diluted enzyme.

3. Prepare the labeling reaction for the control system by adding components in the order listed below. Prepare the sample labeling reaction(s) in the same manner, substituting 5 pmol 3'-OH ends of the sample DNA in place of the Unlabeled Control Oligo.

Note: Mix reactions gently. Do not vortex.

Component	Volume (μL)	Final Concentration
Ultrapure water	25	---
5X TdT Reaction Buffer	10	1X
Unlabeled Control Oligo (1 μM)	5	100nM
Biotin-11-UTP (5 μM)	5	0.5 μM
Diluted TdT (2U/μL)	5	0.2 U/μL
Total Volume	50	---

4. Incubate reactions at 37°C for 30 minutes.
5. Add 2.5 μL 0.2M EDTA to stop each reaction.
6. Add 50 μL chloroform:isoamyl alcohol to each reaction to extract the TdT. Vortex the mixture briefly, then centrifuge 1-2 minutes at high speed in a microcentrifuge to separate the phases. Remove and save the top (aqueous) phase.
7. To determine labeling efficiency, see the Procedure for Estimating Labeling Efficiency on the next page. At this point, the DNA is ready to be used in the end application.

Note: For applications such as electrophoretic mobility shift assays (EMSA) that require biotin-labeled double-stranded DNA, complementary oligos should be end-labeled separately and then annealed before use. Anneal oligos by mixing together equal amounts of labeled complementary oligos and incubating the mixture for 1 hour at room temperature. Oligonucleotides with high melting temperatures or secondary structure may require denaturation and slow cooling for optimal annealing (e.g., denature at 90°C for 1 minute, then slowly cool and incubate at the melting temperature for 30 minutes). Freeze annealed oligos that will not be used immediately, and thaw on ice for use. Removal of the unincorporated Biotin-11-UTP is not necessary for use in EMSA but may be necessary for other applications.

Procedures for Estimating Labeling Efficiency

Labeling efficiency can be determined by dot blots using either a dot/slot blotting apparatus (Option 1) or by hand spotting (Option 2). The following dot blot protocols were developed for use with the detection reagents in the LightShift[®] Chemiluminescent EMSA Kit (Product No. 20148). Sample results appear in the Appendix of these instructions.

A. Additional Materials Required

- Positively-charged nylon membrane (e.g., Biodyne[®] B Membrane, Product No. 77016)
- Dot blotting apparatus
- TE Buffer: 10mM Tris•HCl, 1mM EDTA, pH 8.0
- 96-well microplate (low adsorption) for preparing dilutions
- Multi-channel pipette
- Microcentrifuge tubes and microcentrifuge
- UV lamp or cross-linking device equipped with 254nm bulbs or 312nm transilluminator
- Streptavidin-HRP and chemiluminescent substrate reagents (as in LightShift Chemiluminescent EMSA Kit, Product No. 20148)
- X-ray film or CCD camera

B. Option 1: Dot Blot Using a Dot/Slot Blotting Apparatus

1. Hydrate/equilibrate a positively-charged nylon membrane in TE Buffer for at least 10 minutes.
2. Pipette 125 μ L TE Buffer into wells B1 through H12 of a 96-well dilution plate (leave wells A1-A12 empty).
3. Dilute a sample of the Biotin Control Oligo and the Unlabeled Control Oligo stocks 200-fold in TE Buffer to make 5 nM oligo working stocks (e.g., 2 μ L Control Oligo + 398 μ L TE Buffer).
4. In microcentrifuge tubes, prepare a series of oligo standards according to the following table:

Component	% Biotin				
	100	75	50	25	0
Biotin Control Oligo (5 nM)	15	11.25	7.5	3.75	0
Unlabeled Control Oligo (5 nM)	0	3.75	7.5	11.25	15
TE Buffer (pH 8.0)	285	285	285	285	285
Total Volume	300 μ L				

5. Pipette 250 μ L of the above oligo standards into wells A1-A5 of the 96-well microplate.
6. In a microcentrifuge tube, prepare a 20-fold dilution of the test TdT labeling reaction in TE Buffer to achieve a final concentration of 5nM (e.g., 2 μ L TdT reaction + 38 μ L TE Buffer).
7. In another microcentrifuge tube, combine 15 μ L of 5nM dilution from Step 6 with 285 μ L TE Buffer. Pipette 250 μ L of this sample into an available "A" well in the unused portion (A6-A12) of the 96-well microplate above.
8. Prepare a series of two-fold dilutions of standards and samples by removing 125 μ L aliquots from all "A" wells and mixing them with the TE Buffer in corresponding "B" wells, continuing down the plate through the "H" wells.
9. Place the hydrated nylon membrane into the dot blot apparatus. Add 100 μ L TE into wells of dot blotting apparatus.
10. Apply vacuum or attach to a peristaltic pump to establish a flow rate of 100 μ L/~5 min/well.
11. When the solution has been drawn through the membrane, break the vacuum to stop flow.
12. Apply 100 μ L per well of samples from the microplate (results in 25 fmol 3'-OH ends in spot A to 0.2 fmol in spot H).
13. Apply vacuum to draw samples through the membrane.
14. Wash wells three times with 125 μ L TE Buffer, breaking the vacuum between each application.
15. After the final wash, remove the membrane from the blotting device and place it on a clean paper towel. Allow the residual buffer to absorb into the membrane.
16. Immediately UV crosslink the membrane as described in Section D below.

C. Option 2: Dot Blot by Hand Spotting

Note: The same quantity of DNA per spot will be applied as in Option 1 but in a smaller total volume.

- Hydrate/equilibrate a positively-charged nylon membrane in TE Buffer for at least 10 minutes.
- Dilute a sample of the Biotin Control Oligo and the Unlabeled Control Oligo stocks 20-fold in TE Buffer to make 50nM oligo working stocks (e.g., 2 μ L Control Oligo + 38 μ L TE, pH 8.0).
- In microcentrifuge tubes, prepare a series of oligo standards according to the following table:

Component	% Biotin				
	100	75	50	25	0
Biotin Control Oligo (50 nM)	12	9	6	3	0
Unlabeled Control Oligo (50 nM)	0	3	6	9	12
TE, pH 8.0	48	48	48	48	48
Total Volume	60 μ L				

- Pipette 50 μ L of the oligo working stocks into wells A1-A5 of a 96-well dilution plate.
- In a microcentrifuge tube, make a 10-fold dilution of the test TdT labeling reaction in TE Buffer to achieve a final concentration of 10nM (e.g., 6 μ L TdT reaction + 54 μ L TE, pH 8.0).
- Place 50 μ L of each 10nM test DNA samples into unused "A" wells of the 96-well plate. Prepare a series of two-fold dilutions of standards and samples by removing 25 μ L aliquots from all "A" wells and mixing them with the 25 μ L TE Buffer in corresponding "B" wells, continuing down the plate through the "H" wells.
- Place the equilibrated membrane onto a clean, dry paper towel. Allow excess buffer to absorb into the membrane, but do not allow the membrane dry out.
- Spot 2 μ L of samples and standards onto the membrane (resulting in 20 fmol 3'-OH ends in "A" spots and 0.16 fmol in "H" spots). Allow the samples absorb into the membrane.

D. UV Crosslink the Dot blot

- Immediately UV crosslink the membrane by one of the following three methods:
 - Option 1:** Crosslink at 120mJ/cm² using a commercial UV-light crosslinking instrument equipped with 254nm bulbs (45-60 second exposure using the auto crosslink function).
 - Option 2:** Crosslink at a distance of approximately 0.5cm from the membrane for 5-10 minutes with a hand-held UV lamp equipped with 254nm bulbs.
 - Option 3:** Crosslink for 10-15 minutes with the membrane face down on a transilluminator equipped with 312nm bulbs.
- Continue with the detection and analysis immediately, or store the membrane dry at room temperature until the detection protocol can be performed.

E. Detection and Analysis



Detect the spotted standards and samples using the procedure and reagents for the LightShift Chemiluminescent EMSA Kit (Product No. 20148) or Chemiluminescent Nucleic Acid Detection Module (Product No. 89880). To determine the labeling efficiency, compare spot intensities of the sample lanes to those of the Biotin Control Oligo standards.

- If using X-ray film to document results, compare the row of sample spots to the row of standard spots to estimate efficiency. Densitometry of the film also can be performed.
- If using a cooled CCD camera to document results, spot densitometry can be performed (choose a dilution that is within the linear exposure range) and a standard curve constructed from which to extrapolate the labeling efficiency of the unknown samples.

The Unlabeled Control Oligo should be labeled with > 70% efficiency as determined by the dot blot analysis described here. The efficiency of TdT labeling is somewhat variable, even among different single-stranded oligonucleotides. This variability does not correlate directly to the identity of the 3' terminal base, but is related to the overall sequence. Typically, oligonucleotides with relatively inefficient labeling (< 50%) still produce good signal in subsequent chemiluminescent EMSA detection procedures.

Appendix

A sample dot blot to estimate labeling efficiency appears below. The blot includes the dilution series for each of the standards made in Option 1 of the Procedures for Estimating Labeling Efficiency as well as three different test oligos. A dot blotting apparatus and vacuum were used to spot the samples. The blot was detected using the reagents supplied in the LightShift Chemiluminescent EMSA Kit (Product No. 20148).

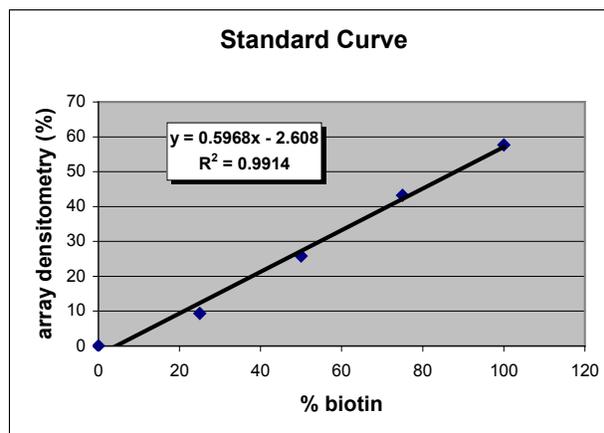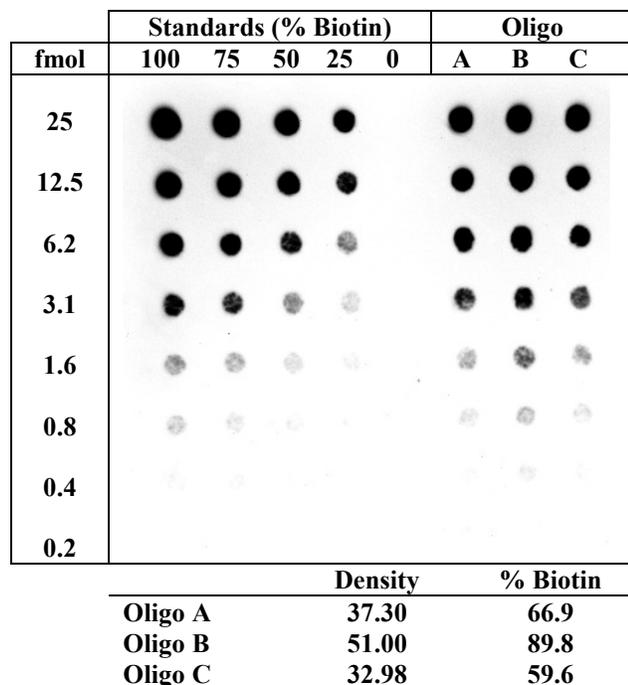

Related Thermo Scientific Products

20148	LightShift Chemiluminescent EMSA Kit
89880	Chemiluminescent Nucleic Acid Detection Module
77016	Biodyne [®] B Nylon Membranes, 8 × 12 cm, 25 sheets, positively charged with 0.45 μm pore size
78833	NE-PER [®] Nuclear and Cytoplasmic Extraction Reagents
17097	North2South [®] Chemiluminescent Hybridization and Detection Kit
17075	North2South [®] Biotin Random Prime DNA Labeling Kit

Cited References

- Roychoudhury, R. and Wu, R. (1980). Terminal transferase-catalyzed addition of nucleotides to the 3' Termini of DNA. *Methods Enzymol* **65**:43-62.
- Roychoudhury, R., et al. (1976). Terminal labeling and addition of homopolymer tracts to duplex DNA fragments by terminal deoxynucleotidyl transferase. *Nucl Acids Res* **3**:863-77.
- Michelson, A.M. and Orkin, S.H. (1982). Characterization of the homopolymer tailing reaction catalyzed by terminal deoxynucleotidyl transferase. *J Biol Chem* **257**:14773-82.

Product Reference

Cornelussen, R.N.M., et al. (2001). Regulation of prostaglandin A1-induced heat shock protein expression in isolated cardiomyocytes. *J Mol Cell Cardiol* **33**:1447-54.

Biodyne® is a registered trademark of Pall BioSupport Corporation.

This product ("Product") is warranted to operate or perform substantially in conformance with published Product specifications in effect at the time of sale, as set forth in the Product documentation, specifications and/or accompanying package inserts ("Documentation") and to be free from defects in material and workmanship. Unless otherwise expressly authorized in writing, Products are supplied for research use only. No claim of suitability for use in applications regulated by FDA is made. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the Product is subjected to normal, proper and intended usage. This warranty does not extend to anyone other than the original purchaser of the Product ("Buyer").

No other warranties, express or implied, are granted, including without limitation, implied warranties of merchantability, fitness for any particular purpose, or non infringement. Buyer's exclusive remedy for non-conforming Products during the warranty period is limited to replacement of or refund for the non-conforming Product(s).

There is no obligation to replace Products as the result of (i) accident, disaster or event of force majeure, (ii) misuse, fault or negligence of or by Buyer, (iii) use of the Products in a manner for which they were not designed, or (iv) improper storage and handling of the Products.

Current product instructions are available at www.thermoscientific.com/pierce. For a faxed copy, call 800-874-3723 or contact your local distributor.

© 2011 Thermo Fisher Scientific Inc. All rights reserved. Unless otherwise indicated, all trademarks are property of Thermo Fisher Scientific Inc. and its subsidiaries. Printed in the USA.